


SGR540/541/542 Series

Advanced Digital

Rotary Torque Transducer

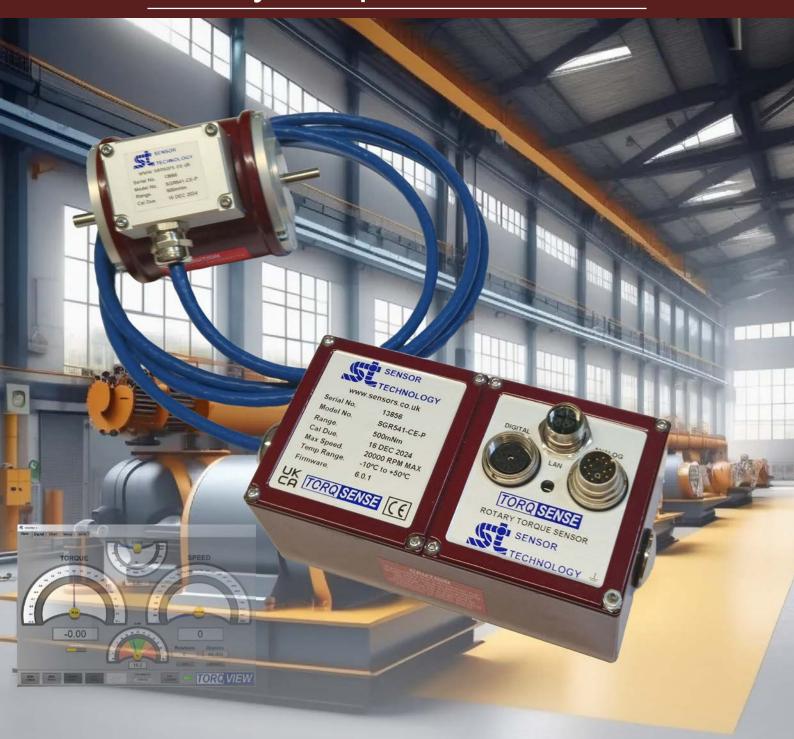

Website: www.omniinstruments.co.uk

Tel: +44 (0) 1382 443000 Email: info@omni.uk.com



TORQ SENSE

Digital SGR540/541/542 series Torque Transducer

Torqsense Digital rotary strain gauge series (SGR) Transducers with separate electronics, use non contact technology eliminating the need for noisy slip rings. They are suitable for torque measuring, testing, feedback control of drive mechanisms and process control applications.

The SGR series transducers use modern strain gauge signal conditioning techniques to provide a high bandwidth low cost torque measuring solution with high overrange and overload capabilities.

Benefits & Features

- Transducers from 175mNm to 13000 Nm.
- Large fully functional overrange capability of 250%
- Separate digital electronics
- Minimal side and end load errors
- Low linearity deviation of ± 0.05 % FSD
- Low hysteresis error of ± 0.05 % FSD
- Zero variation in torque signal with rotation (cyclic variation)
- Non contact signal transmission, no slip rings to wear out
- High digital sample rate of 4000 samples per second
- Adjustable torque data smoothness, low pass filter
- Speed measurement / Angle / Power computation
- Wide power supply range 12-32 VDC
- Optional integrated Ethernet allows a transducer to be accessed by multiple users simultaneously, from anywhere the connected network reaches.

Technology

The SGR series torque transducers use a full four element strain gauge bridge to measure the torsion present on a shaft. The full bridge helps to diminish errors from any off-axis forces that are sometimes unintentionally applied to the transducer in some test setups. The full bridge also increases the sensitivity and the temperature performance of strain measurement.

A rotor mounted ultra-miniature microcontroller measures the strain gauge bridge and transfers the information back to the stator digitally eliminating any noise pickup usually associated with slip ring and other analog methods of transferring torque data from rotor to stator. External noise pickup into the gauge wiring is virtually eliminated due to the short distance between the strain gauge elements and the rotors measuring circuits.

A multipoint calibration method reduces any linearity errors within the sensor. A large functional overrange capability allows the peaks of a torque signal to be captured more faithfully without any clipping when operating the sensor close to its full scale rating.

All this combined with a mechanical overload capability of over 400% make the SGR series torque sensors a very robust and accurate torque measuring solution.

TorqSense SGR540/541/542 transducers offer:

- **SGR540** Torque measurement only
- **SGR541** Torque, speed & power measurement (60 pulses per revolution encoder)
- **SGR542** Torque, speed/angle & power measurement (360 pulses per revolution incremental encoder)
- BIT Self-diagnostics Diagnostic system checks internal systems and operational conditions for faults, and monitors torque, speed and temperature for overscale conditions.
- Transducer status LED and simple "Sensor status" output pin, provide transducer health feedback.
- Sensors to monitor shaft temperature for better compensation and accuracy.
- Digital outputs RS232 and USB (standard), CAN Bus and Ethernet (optional).
- Transducer Control configuration software is provided to setup and configure the transducer.
- 3 analog channels are individually configurable, allowing changes to scaling and data assignment.
- Ability to connect up to 10 transducers using USB.
- Optional integrated Ethernet provides distributed access and multiple simultaneous user/device use.

TORQ VIEW Software

TorqView is an easy to use advanced torque monitoring software, available to assist data recording and instrumentation displays that interface with Windows based PCs.



LabView VI's are available for users to design their own process control applications. DLLs are also available for users to write their own custom software. Get data from across your network using the ethernet module.

Omni Instruments Ltd


Website: www.omniinstruments.co.uk

| Parameter | Condition Data U | | | | | | | | Units | | |
|---|----------------------|---|-----------------------------|------------|-----------------------------|---------|------------------------------|------------------------------------|---------------|-------------------------------------|---------|
| SGR540/541/542 Torque i | measurement | system | | | | | | | | | |
| Measurement method | neasurement | зузтепт | | | Full bridge | strair | n dalide | | | | |
| Wedsarement metrod | | | 0 – 1 | .1 | 0 – 21 | | - 101 | 0 - 501 | | 0 - 2001 | |
| Torque range | (Natas 1 8 2) | 0 – 1 | to 0 - | | 0 - 100 | | 0 - 500 | to 0 - 200 | | 0 - 13000 | Nm |
| Torque range | (Notes 1 & 2) | [0 - 10] | | | 0 – 201 0 - 1000] | | - 1001 0 - 50001 | [0 - 500 to 0 - 2000 | | 0 - 20001 0 - 175000] | [lbfin] |
| Shaft size (diameter) | | 6 | 12 | | 20 | | 30 | 50 | | 75 | mm |
| Specifications | | | | | | | | | | | |
| Combined non-linearity and hysteresis | | | | | | ±0.1 | l | | | | %FS |
| Resolution | | | | | | 0.01 | | | | | %FS |
| Repeatability | | | | | | 0.05 | 5 | | | | %FS |
| , | 20°C, SM | | | | | ±0.1 | ı | | | | %FS |
| Accuracy | (Note 4) | | | 1 | | ±0.1 | | | 1 | | |
| Digital averaging | (Note 5) | 2 | 4 | 8 | 16 | | 32 | 64 | 128 | 256 | N |
| Noise Floor | 20°C, SM (Note 4) | 0.06 | 0.04 | 0.03 | 0.02 | | 0.015 | 0.01 | 0.01 | 0.01 | %FS |
| 3dB Bandwidth | (Note 6) | 2000 | 1000 | 500 | 250 | | 125 | 62 | 31 | 15 | Hz |
| Analog output | | | | | | | | | | | |
| Output voltages | | | , | | | | ±5 / ±10 / | | , | | Vdc |
| (Torque/Speed/Power) | | | (| SGR540 Se | | | | er selectable | 2) | | |
| Load impedance | | | | Ont | | aximu | | / 12 . 0 | | | ΚΩ |
| Output currents (Torque/Speed/Power) | | | (| | | | -20 / 0-20 / ents are us | / 12±8 er selectable | ·) | | mA |
| 4-20mA Loop resistance | | | (| 0011070 00 | | | ceed 400 | or sciectable | ′/ | | Ω |
| Digital output | | | | | 0110414 | | 10004 100 | | | | |
| Connections | | CAN | Bus | Et | hernet | | RS232 | | | USB | |
| | | CAN 2.0B, 11bit Message Identifiers | | IEEE 802.3 | | | Data Bits: 8, | | | | |
| Configuration | | | | | 10BASE-T, 100BASE-TX | | Parity: None, Stop Bits:1 | | USB 2.0 | Full-Speed | |
| | | | | | Mbps, | | 11520 | | | | |
| Baud Rate(s) | | 250Kbps, | | | 0Mbps | | | , 9600bps | 12 | Mbps | |
| Output Rate | (Note 7) | Up to 4 kHz Up to 1.9 kHz Up to 1.1 kHz Up to 4kHz | | | | | | to 4kHz | | | |
| Rotation speed/angle of ro | otation measu | rement syst | tem | | | | | | | | |
| Measurement method | | | | | | | gh slotted | | | | |
| Direct output signal | | | | | | pto sv | | 5V square v | | | |
| Accuracy | | | ed: ±1rpm ι | | | L | | gle: ±1° <i>(36</i> 6 | | only) | |
| Rotational speed (max) | (Note 3) | 30,000 | l . | ,000 | 15,000 | | 12,000 | 9,0 | | 6,000 | RPM |
| Digital Processing | | | essing Met | | Uŗ | odate | rate for a | analog and | digital ou | ıtputs | |
| Techniques Processing modes run | Based on a | | 1 (Slow Met | | | | | 1 | | | Hz |
| simultaneously and can be | standard | Fre | quency Cou | It | 0 RP | NA | | | 1 | | |
| applied to either analog | 60-line | Mada | 2 (Fast Met | hod) | URP | IVI | | | | | - |
| channel or accessed | grating. | | 2 (Fast Met) eriod Count | iiou) | > 0 R | PM | | | RPM_ RPM_, | | Hz |
| individually via a digital connection. | (Note 11) | , | | | × 0 K | 141 | | [= | 1000 | | |
| Temperature | | | | | | | | | | | |
| Temperature accuracy | | | | | | ±1 | | | | | °C |
| Reference temperature T _{RT} | | | | | | 20 | | | | | °C |
| Compensated range, ΔT ₀ | | | | | (|) to + | | | | | °C |
| Usable range, ΔT _S | | | | | | 10 to - | | | | | °C |
| Temperature | | | | | | | | | | | % |
| Temperature | | Coefficient of zero 0.002 Coefficient of span 0.01 | | | | | | | % | | |
| Power supply | | | | | | | | | | | |
| Nominal voltage, Vs | | | | | 12 1 | to 32 (| (max) | | | | V |
| Current consumption, Is | | 12 to 32 (max) 250 (max) @ 12 VDC | | | | | | | mA | | |
| Power consumption, W _S | | | 250 (max) @ 12 VDC | | | | | | | | W |
| Allowed residual ripple of | | | | | | 500 |) | | | | |
| supply voltage, V _{ripple} | | | | (| above nom | | upply volta | ge) | | | mVp-p |
| Electromagnetic compatible | ility | | | | | | | | | | |
| EMC compatibility | | | | | EN d | 61326 | :2006 | | | | |
| | | | | | | | | | | | |

^{*} For notes, please see glossary page

Omni Instruments Ltd Tel: +44 (0) 1382 443000 Email: info@omni.uk.com Website: www.omniinstruments.co.uk


Dimensions (1Nm to 100Nm)

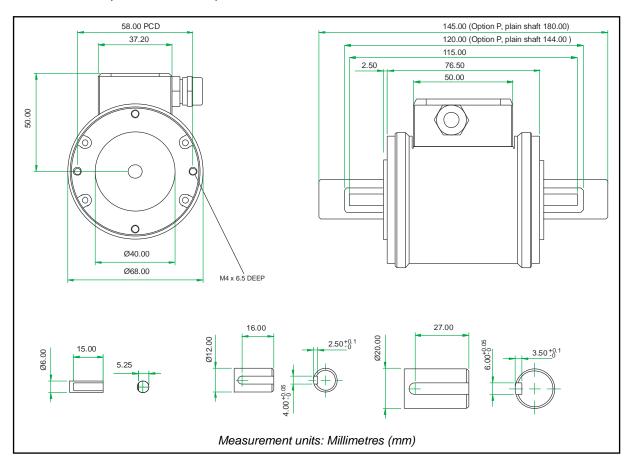

| Parameter | | _ | _ | _ | _ | _ | Data | _ | _ | _ | _ | _ | _ | _ | Units |
|---|-----------------------|-------|------|------|-------|------|------|------|-------|------|------|------|------|------|--|
| Parameter | | | | | | | Data | | | | | | | | UTITES |
| Mechanical Properties | | | | | | | | | | | | | | | |
| Torque (Max) | 0.225 | 0.6 | 1 | 2.5 | 3.5 | 6 | 8.5 | 13 | 17.5 | 20 | 30 | 55 | 85 | 100 | Nm |
| Shaft Code | CD | CE | CF | DA | DF | DB | DC | DG | DD | DE | EB | EC | ED | EE | |
| Standard Shaft Type | Plain | Plain | Flat | | | | | | Keyed | | | | | | |
| Shaft Size (Diameter) | | 6 | | | 12 20 | | | | | | | mm | | | |
| Torsional Stiffness | 0.23 | 0.23 | 0.23 | 1.28 | 1.3 | 1.32 | 1.6 | 1.7 | 1.8 | 1.9 | 4.1 | 6.4 | 8.1 | 9.2 | KNm/rad |
| Mass moment of inertia, L _V | 0.45 | 0.45 | 0.45 | 5.96 | 6.00 | 6.04 | 6.13 | 6.18 | 6.24 | 6.42 | 22.9 | 23.9 | 25.4 | 27.2 | ×10 ⁻⁶ kg·m ² |
| Max measurable load limit | 250 (of rated torque) | | | | | | | | % | | | | | | |
| Static safe load breaking | 400 (of rated torque) | | | | | | | | % | | | | | | |
| Shaft weight, approx | 0.03 | 0.03 | 0.03 | 0.14 | 0.14 | 0.14 | 0.14 | 0.15 | 0.15 | 0.15 | 0.36 | 0.37 | 0.40 | 0.41 | kg |
| Transducer with shaft weight, approx | 0.7 | 0.7 | 0.7 | 0.8 | 0.8 | 0.8 | 0.8 | 0.8 | 0.8 | 0.8 | 1.0 | 1.0 | 1.1 | 1.1 | kg |

Omni Instruments Ltd Tel: +44 (0) 1382 443000 Email: info@omni.uk.com Website: www.omniinstruments.co.uk


Dimensions (101Nm to 500Nm)

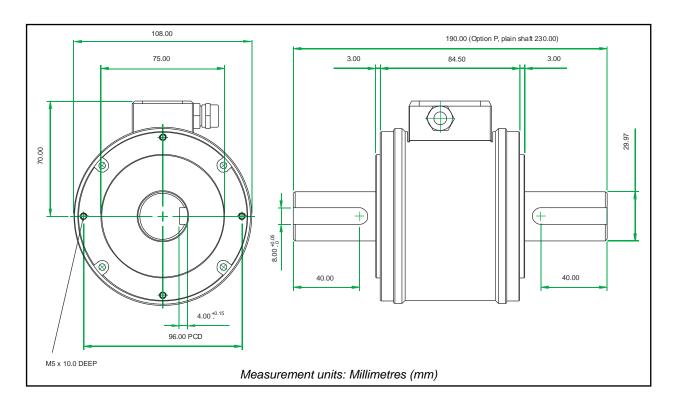

| Parameter | | Units | | | | |
|---|--------|-------|-------|-------|-------|---|
| Mechanical Prope | erties | | | | | |
| Torque (Max) | 175 | 225 | 265 | 350 | 500 | Nm |
| Shaft Code | FA | FB | FC | FD | FE | |
| Standard Shaft Type | | | Keyed | | | |
| Shaft Size (Diameter) | | mm | | | | |
| Torsional stiffness | 32.9 | 35.6 | 37.2 | 37.9 | 39.8 | kNm/rad |
| Mass moment of inertia | 138.9 | 143.1 | 147.7 | 151.9 | 174.2 | ^x 10 ⁻⁶ kg·m ² |
| Max measurable load limit | | % | | | | |
| Static safe load breaking | | % | | | | |
| Shaft weight, approx | 1.1 | 1.1 | 1.1 | 1.2 | 1.2 | kg |
| Transducer with shaft weight, approx (1 dp) | 2.3 | 2.3 | 2.3 | 2.4 | 2.4 | kg |


Omni Instruments Ltd Tel: +44 (0) 1382 443000 Email: info@omni.uk.com Website: www.omniinstruments.co.uk

Dimensions (501Nm to 13000Nm)

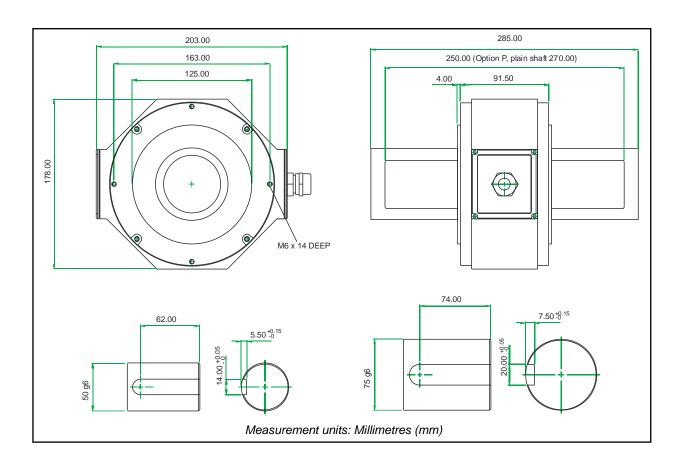

| Parameter | Data | | | | | | | | Units | | | | |
|--------------------------------------|-----------------------|-----|-------|------|-------|----------|----------|--------|-------|------|--------|-------|--|
| | | | | | | | | | | | | | |
| | | | | | Me | chanical | Properti | ies | | | | | |
| Torque (Max) | 650 | 850 | 1100 | 1350 | 2000 | 3000 | 4000 | 6000 | 7000 | 8000 | 10000 | 13000 | Nm |
| Shaft Code | GE | GA | GB | GC | GD | HA | HB | HC | HD | HE | HF | HG | |
| Standard Shaft Type | Keyed | | | | | | | | | | | | |
| Shaft Size (Diameter) | 50 75 | | | | | | | mm | | | | | |
| Torsional Stiffness | TBC | TBC | 199.2 | TBC | 214.1 | TBC | TBC | 914.4 | TBC | TBC | 945.5 | TBC | kNm/rad |
| Mass moment of inertia | TBC | TBC | 1330 | TBC | 1497 | TBC | TBC | 7932.7 | TBC | TBC | 9407.1 | TBC | ×10 ⁻⁶ kg·m ² |
| Max measurable load limit | 250 (of rated torque) | | | | | | | | % | | | | |
| Static safe load breaking | 400 (of rated torque) | | | | | | | % | | | | | |
| Shaft weight, approx | TBC | TBC | 3.9 | TBC | 4.1 | TBC | TBC | 10.2 | TBC | TBC | 10.6 | 11.2 | kg |
| Transducer with shaft weight, approx | TBC | TBC | 7.1 | TBC | 7.3 | TBC | TBC | 13.4 | TBC | TBC | 13.8 | 14.4 | kg |

Website: www.omniinstruments.co.uk

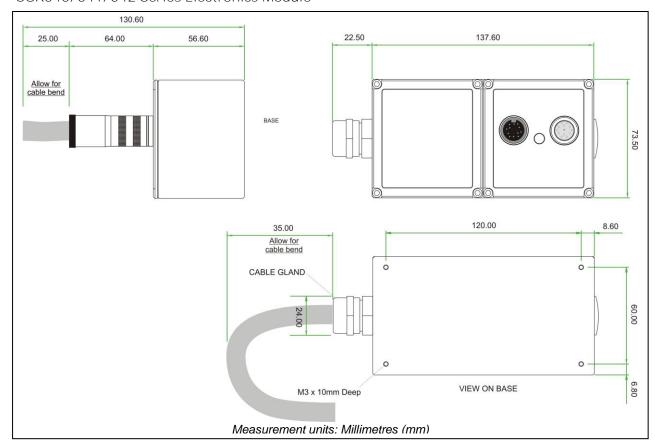

Website: www.omniinstruments.co.uk

• - Standard feature ♦ - Optional feature


| | SGR540/541/542 | Option Code | Remarks / Purpose |
|--|----------------|----------------|---|
| Torque, Speed, Power Outputs | | | |
| Torque only | 540 | | |
| Torque & Speed (60 pulses/rev) or Power | 541 | | Outputs are user selectable |
| Torque & Speed (360 pulses/rev) or Power | 542 | | |
| Standard features | | | |
| Keyed Shaft Ends | • | K | 1Nm will have flats |
| Voltage outputs from ±1v to ±10v FSD and unipolar (Variable) | • | | Output is user selectable |
| USB 2.0 full speed 12 Mbps Digital output | • | | |
| RS232 output | • | | |
| Torque Averaging and Torque Peak | • | | |
| Self Diagnostics | • | | |
| Internal temperature measurement | • | | |
| Deep grooved shielded bearings with oil lubrication | • | | |
| Ingress Protection (IP) 54 | • | | |
| Optional features | | | |
| Plain Shaft Ends | ♦ | Р | Shaft length will be longer than keyed end shafts – consult factory for length |
| Splined Shaft Ends | ♦ | Т | Consult factory for details |
| Current output 0-20mA, 4-20mA & 12±8mA (Variable) | ♦ | F | Current output is user selectable and in place of Voltage output. However user can reselect a Voltage output, if required. (Note 8) |
| CAN Bus output | ♦ | Н | In place of RS232 output |
| Integrated Ethernet | ♦ | 1 | |
| High Speed Bearings (See Note 9 below) | ♦ | J | Concult factory for mayimayim |
| Sealed Bearings | ♦ | S | Consult factory for maximum speed allowance. |
| Ingress Protection (IP) 65 (See Note 10 below) | ♦ | L | specu allowalice. |

SGR540/541/542 Series Torque Transducers - Additional related products

| Code | Remarks/Purpose |
|-------|----------------------------|
| ETD | Display readout |
| PSU 1 | For providing 12-32Vdc |
| SBU 1 | |
| TV | Torque Monitoring Software |
| _ | ETD PSU 1 |

Omni Instruments Ltd Tel: +44 (0) 1382 443000 Email: info@omni.uk.com

| | SGR540/541/542 | Option Code | Remarks/Purpose |
|--|----------------|----------------|---|
| Connectors & Leads | | | |
| Analog Connector 12 Pin Lumberg (female) | ♦ | ACC 1 | For user to self wire |
| Digital Connector 12 Pin Lumberg (male) | ♦ | ACC 2 | For user to self wire |
| Analog Lead (Length 2.5m) 12 Pin Lumberg (female) to 15 way 'D' type connector (female) | ♦ | ACC 3 | For connecting SGR to user's system via 15 pin 'D' connector |
| Digital Lead (Length 2.5m) 12 Pin Lumberg (male) to 15 way 'D' type connector (male) | ♦ | ACC 4 | For connecting SGR to user's system via 15 pin 'D' connector |
| Digital Lead Adapter (Length 1m) 15 Way 'D' type (female) to RS232 and Power Connectors | ♦ | ACC 5 | For connecting SGR to PC via RS232 [Also needs Digital Lead (ACC4) to connect to SGR] |
| Digital Lead Adapter (Length 1m) 15 Way 'D' type (female) to RS232, USB and Power Connectors | ♦ | ACC 6 | For connecting SGR to PC via USB (Option G) or RS232 [Also needs Digital Lead (ACC4) to connect to SGR] |
| Digital Lead Adapter (Length 1m) 15 Way 'D' type (female) to CANbus and Power Connectors | ♦ | ACC 8 | For connecting SGR to PC via CANbus (Option H) [Also needs Digital Lead (ACC4) to connect to SGR] |
| Digital Lead Adapter (Length 1m) 15 Way 'D' type (female) to CANbus, USB and Power Connectors | ♦ | ACC 9 | For connecting SGR to PC via USB (Option G) or CANbus (Option H) [Also needs Digital Lead (ACC4) to connect to SGR] |
| Ethernet cable (Length 2M) | ♦ | ACC 12 | Connecting SGR to LAN |
| Ethernet cable (Length 5M) | ♦ | ACC 13 | Connecting SGR to LAN |
| Ethernet cable (Length 10M) | ♦ | ACC 14 | Connecting SGR to LAN |

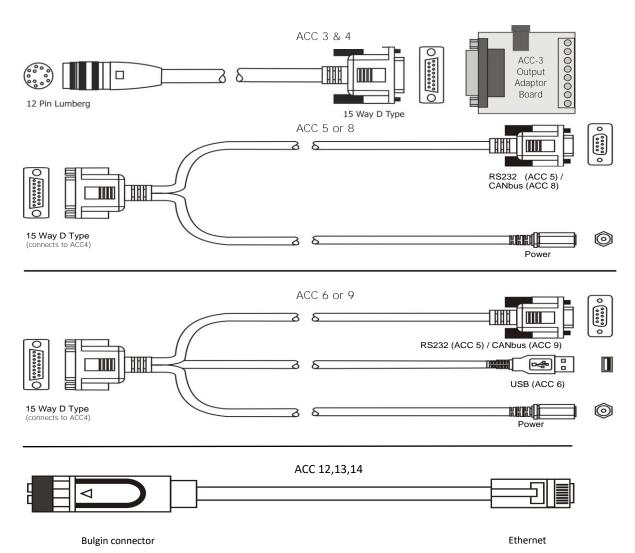

Email: info@omni.uk.com

Tel: +44 (0) 1382 443000

When ordering a Torque Transducer please note that any torque/FSD is possible between ranges — please specify rated torque and options using the following format:

| For example: SGR | 541 - 15Nm - | K-L | A transducer with torque and speed outputs, rated and calibrated to 15Nm FSD with keyed ends and IP65 protection. |
|----------------------------------|--------------|-----|---|
| Your transducer requirement: SGR | | | |
| Max speed (if applicable) | | RPM | |
| Connector or Lead options | | | |
| Additional related products | | | |

Glossary of terms and definitions used in this datasheet

- Accuracy The degree of conformity of a measured or calculated quantity, which will show the same or similar results. Accuracy of the overall TorqSense system is limited by the combined error of several factors such as linearity, hysteresis, temperature drifts and other parameters affecting measurements. If errors in the system are known or can be estimated, an overall error or uncertainty of measurement can be calculated.
- Digital averaging The application of algorithms to reduce white noise. In any electronic system, electronic white noise is mixed with the signal and this noise usually limits the accuracy. To reduce the influence of white noise and increase the accuracy of the system different averaging algorithms can be applied. In the TorqSense system a flying digital averaging technique is applied to reduce the white noise commensurate with the level of accuracy required. However, as any averaging algorithm works as a low pass filter, the more averaging that is applied the lower the frequency response. Therefore, each Torqsense system should be optimised to the customer's requirements by choosing the right combination of accuracy/frequency response. Please see relevant part of the Datasheet and User Manual.
- Note 1: Any torque/FSD is possible between ranges please specify max rated torque.
- Note 2: Max rated torque should not be exceeded.
- Note 3: Please consult factory for applications requiring rotational speeds that exceed maximum figures given. Transducers fitted for IP65 will have running speeds considerably reduced, increased drag torque and accuracy can be affected.
- Note 4: SM Static Mode. Dynamic values will depend upon user application and has to be adjusted accordingly.
- Note 5: Digital averaging can be configured by user to optimise accuracy/frequency response for specific user applications. Digital averaging default setting is N=16. For details see User Manual.
- Note 6: 4kHz approximate sample rate, actual rate may be slightly under.
- Note 7: Output rate figures were calculated from the time taken to capture 100,000 torque readings. Testing was conducted with each connection method configured at its maximum baud rate. Each connection method was tested in isolation on an Intel 7th generation i7 PC running Windows 10. The CAN bus, RS232 and USB interfaces were tested using a stripped-down capture program, while Ethernet was tested via the DLL.
 - USB USB is a host-based bus architecture, because of this the output rate achievable may be affected by other bus traffic and host activity
 - CAN Bus CAN Bus is a shared bus technology, where other bus traffic may affect the maximum output rate achievable.
 - Ethernet Ethernet carries a much greater overhead than the other connection methods. Ethernet can be affected by dropped packets and other network traffic.
 - The digital output rate does not in any way influence the internal sampling rate of the transducer. The internal sampling and digital interfaces run asynchronously; the digital interface merely copies data from a buffer at the requested rate.
- Note 8: 3 x analog channels are available.
 - Default assignments for an SGR540 (torque only) are Channel 0 torque, Channel 1 torque peak, Channel 2 torque auto reset.
 - Default assignments for an SGR54x (torque and speed) are Channel 0 torque auto (torque/torque peak, switched by peak input), Channel 1 speed, Channel 2 power.
 - Voltage/Current scaling set per option selection, or via Transducer Control on advanced models.
- Note 9: At very high speeds, for better balance the factory recommends plain or splined shafts.
- Note 10: Transducers fitted for IP65 will have running speeds considerably reduced, increased drag torque and accuracy can be affected.
- Note 11: The RPM reading update rate is directly related to the square wave frequency produced from a shaft mounted grating passing through an opto switch. The values specified are based on a standard 60-line grating, for models fitted with an angle encoder or different grating size, replace the RPM with the square frequency in Hz. The square wave frequency can be calculated by this formula: SQWaveFrequencyHz = (RPM / 60) x GratingSize (for quadrature-based encoders, double the grating size).

Omni Instruments LtdTel: +44 (0) 1382 443000Website: www.omniinstruments.co.ukEmail: info@omni.uk.com